

CLEANING AND MAINTENANCE

Check whether the battery level is sufficient before each use. If the battery is low (display shows battery icon) change the batteries and then take the temperature.

Before each use, check the equipment casing for damage. If it is damaged, do not use.

Wipe with a soft, dry cloth after each use. If the thermometer is dirty, you may wipe the unit with a damp cloth moistened with water or neutral detergent and then wipe it with a dry cloth. Avoid water entering the body of the thermometer, so that the internal electronic components do not get damaged.

This no-contact thermometer does not require disinfection. If you are concerned about contamination, however, you may clean the thermometer with 75% alcohol before and after use.

Do not use volatile oil, paint thinner, and other chemical solvents to wipe the product.

TROUBLESHOOTING AND DISPLAY ERROR MESSAGES

SYMBOL	REASON	SOLUTION
	Battery voltage is too low	Replace battery as soon as possible
	System error	Contact your local dealer
	Measured temperature is too high	Stop measurement
	Measured temperature is too low	Stop measurement

CLASSIFICATION

- Internally powered equipment
- Type BF applied part: Probe
- IP22
- Not category AP / APG equipment
- Mode of operation: continuous operation

KEY TO SYMBOLS

	Indicates a hazardous situation which, if not avoided, could result in death or serious injury
	Indicates a hazardous situation which, if not avoided, may result in minor or moderate injury
	Addresses practices not related to personal injuries, such as product and/or property damage
	Do not dispose of this product in municipal waste. Collection of such waste separately for special treatment is necessary
	Refer to instruction manual/booklet
IP22	Degree of protection against harmful ingress of particulate matter and water.
	Manufacturer
SN	Serial number
	The package should be protected from rain
	The package contains fragile products; please handle with care
	Transport package should be upright
	The maximum stacking layer of the same package; 5 means the layer limit

PRODUCT SPECIFICATIONS

Measure range:	89.6°–109.4°F (32°–43°C)
Accuracy:	±0.4°F, 96.8°–102.2°F (±0.2°C, 36°–39°C), outside the range: ±0.5°F (±0.3°C)
Resolution:	0.1°F/0.1°C
Unit:	°F/°C (the default unit is °F/0.1°F)
Measure time:	1 second
Measure distance:	0–2 inch from the center of forehead between the eyebrows
Memory:	32 sets memories
Work environmental:	Temperature 50°–104°F (10°–40°C) Relative humidity ≤ 85%RH Atmospheric pressure 70–106KPa
Storage environmental:	Temperature: -4°–+131°F (-20°–+55°C) Relative humidity ≤93%RH Atmospheric pressure 70–106KPa
Power	AA(1.5Vx2),d.c.3V
Product size	109.6mm x 44mm x 152.9mm
Product weight	95g (not including batteries)

THREE YEAR LIMITED WARRANTY (CANADA ONLY)

Conair will (at our option) repair or replace your appliance free of charge for 36 months from the date of purchase if the appliance is defective in workmanship or materials. To obtain service under this warranty, return the defective product to the service centre listed below, together with your purchase receipt. In the absence of a purchase receipt, the warranty period shall be 36 months from the date of manufacture.

ANY IMPLIED WARRANTIES, OBLIGATIONS OR LIABILITIES, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE, SHALL BE LIMITED IN DURATION TO THE 36 MONTH DURATION OF THIS WARRANTY. IN NO EVENT SHALL CONAIR BE LIABLE FOR ANY SPECIAL, INCIDENTAL OR CONSEQUENTIAL DAMAGES FOR BREACH OF THIS OR ANY OTHER WARRANTY, EXPRESS OR IMPLIED, WHATSOEVER.

This warranty gives you special legal rights, and you may also have other rights which vary from province to province.

CONAIR CONSUMER PRODUCTS ULC

SERVICE CENTRE:

Conair Consumer Products ULC
100 Conair Parkway, Woodbridge, ON L4H 0L2
ITH93C

For more information on any Conair Products call:
1-855-926-6247
Visit our Web site: www.conaircanada.ca

©2020 Conair Consumer Products ULC
100 Conair Parkway, Woodbridge, ON L4H0L2

HAVE A QUESTION?

Please do not return this product to the retailer.

CALL US FIRST!

Our customers service and product experts are ready to answer ALL your questions. Please call our TOLL-FREE customer service number at: 1-855-926-6247 Or visit us online at www.conaircanada.ca

Consumer Call Centre E-mail:
Consumer_Canada@Conair.com

Belter model number TE-93

Shenzhen Belter Health Measurement and Analysis Technology Co.,Ltd.
702/704, Block C,
Tsinghua Unis Science
No.13 Langshan Rd,
Hi-Tech Industrial Park(north), Nanshan District, 518057
Shenzhen
People's Republic of China

20PG0010CL

IB-20/311

INFRARED THERMOMETER FOREHEAD



Instruction Booklet

For your safety and continued enjoyment of this product, always read the instruction booklet carefully before using.

CONAIRCARE®

Model ITH93C

Thank you for purchasing the ConairCare Infrared Forehead Thermometer (ITH93C). This product features the latest technology and has been tested according to international medical device standards for home and professional use. The thermometer's unique technology enables stable and accurate measurements every time. This product is designed specifically to monitor body temperature for use at home or in clinical settings.

Please read the instruction manual carefully and keep it in a safe place for reference.

INDICATIONS FOR USE

The ITH93C is a non-sterile, reusable, clinical electronic thermometer using an infrared sensor to detect human body temperature on people of all ages for home and professional use.

WARNINGS & PRECAUTIONS

Never use the thermometer for purposes other than those it has been intended for.

The use of this thermometer is not intended as a substitute for a consultation with your healthcare provider. If you are concerned about your health, please see your physician. Elevated temperature may signal a serious illness, especially in older individuals, people with compromised immune systems, and infants.

In order to properly diagnose an elevated temperature, it is important to know an individual's normal body temperature. We suggest taking several readings when the person is healthy, to set a baseline for their normal temperature.

Infrared thermometers cannot be used to diagnose COVID-19 or other illnesses. Infrared thermometers can identify individuals with higher than average body temperatures compared to a sample population. Only a medical professional can determine whether an individual is experiencing an abnormal medical condition or illness.

Note that an abnormal medical condition may be present even when an individual does not show a fever. When in doubt, consult your physician.

Follow general safety guidelines when using this thermometer on children. Do not allow children to take their temperature unattended. This is a not toy. We recommend not using this thermometer on children less than 2 years of age.

Do not immerse this thermometer in water or other liquids. Follow the instructions in the "Cleaning and Maintenance" section to clean and disinfect the thermometer.

The device is made of precision parts. Do not dismantle, re-assemble or modify the thermometer in any way. Do not drop the thermometer and protect it from strong impacts.

Do not use this thermometer if the sensor is broken. If the device is broken, do not attempt to repair it yourself. Contact the customer service center.

Do not use this thermometer in the presence of flammable anesthetic mixtures with air or with oxygen or nitrous oxide.

CAUTION

Keep the device away from direct sunlight. Store in a dry and dust-free environment, ideally within a storage temperature range of 4°F to 131°F (-20°C to 55°C).

Before taking temperature readings, please make sure the sensor surface is clean. If there is visible dust or dirt, you may clean the surface with a cotton swab dipped in rubbing alcohol before using the device.

After cleaning the sensor head with alcohol, it is recommended to leave the device for a few minutes until the alcohol evaporates and the sensor head returns to its normal temperature. We suggest cleaning the thermometer sensor after use, to ensure measurement accuracy and to avoid potential cross-contamination.

To make sure the measurement result is accurate, wait at least 30 seconds after each measurement before you measure again.

Because babies are slower at adapting to temperature changes in the environment, if drastic temperature changes are observed, it is best to wait a few minutes

in the same environment until the baby's body temperature becomes stable before taking any temperature readings to ensure the most accurate results.

It is recommended to take 3 temperature readings and reference the highest recorded measurement for babies between 2 years to 3 years of age, or for first-time users of the device.

The device requires no calibration.

Remove batteries if the equipment is not likely to be used for some time.

The user must check that the equipment functions safely and see that it is in proper working condition before use.

Do not operate the product out of operating conditions or out of the operating temperature range, as it may cause measurement value anomalies or malfunction.

HOW THE THERMOMETER WORKS


This thermometer detects infrared energy radiated from the skin and tissue of the forehead. Temperature readings taken in the center of the forehead (between and slightly above the eyebrows) will provide the most accurate measurements. This thermometer has been tested and proven to be safe and accurate when used as directed in this instruction manual. This device has settings that alert you to a temperature above normal.

Normal temperature varies from person to person, by age, and even by time of day and activity. It is best to establish a "normal" temperature range for each user of the thermometer while the person is feeling well. We suggest taking readings in the morning and in the late afternoon and averaging them to get a "normal" temperature. Record that temperature so you can use it to compare against temperatures measured for that person when they are not feeling well. Note that normal body temperatures tend to decrease with age. The ConairCare thermometer allows you to customize your high temperature alert settings depending on your own normal temperature.

Generally, temperatures in the range of 96.4 ° – 99.4°F (35.8-37.4°C) are considered normal, a temperature between 99.5–101.3°F (37.5 °C – 38.5 °C) is considered a light fever and temperatures over 101.3 °F (38.5 °C) are considered a fever.

The ConairCare thermometer features automatic ambient temperature compensation and forehead temperature dynamic compensation.

GETTING TO KNOW YOUR THERMOMETER

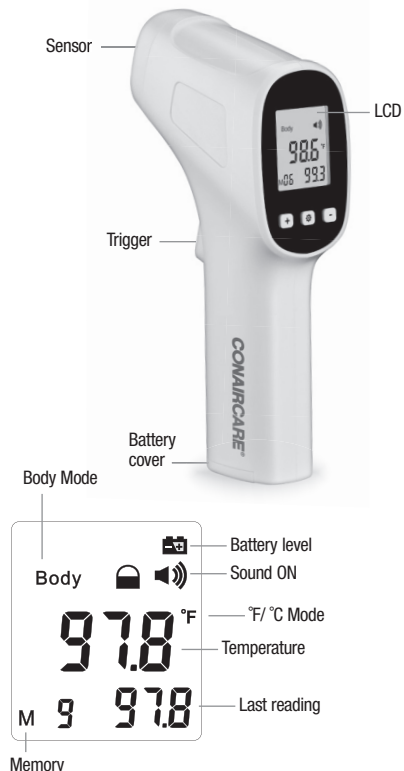

SETTING UP YOUR THERMOMETER

Press trigger button on the handle to turn on device. If the thermometer display does not light up, open the battery door on the bottom of the handle and make sure the batteries are correctly installed with respect to polarity. Close the battery door and press the button again. The display will light up. When the thermometer is turned on and the display lit, press and hold the "⚙️" key to enter the function settings.

1. Selecting temperature units

The screen will display F1 and then show the temperature unit (°F/°C). The default is °F. To change to °C, press the "+" button. To change back to °F, press the "-" button. Press "⚙️" to advance to the fever alert setting.

2. Setting the fever alert

The screen displays F2 and then shows the current fever alert temperature. The default setting is 99.1 °F. To increase the threshold, press the "+" button. To decrease the threshold, press the "-" button. Press "⚙️" to advance to the temperature offset value setting.

3. Setting the temperature offset value

The screen displays F3 and then shows the offset value. The default setting is 0.0 °F/°C. Press "⚙️" to leave temperature offset in the default setting or "+" to increase or "-" to decrease. Then press "⚙️" to enter the auditory alert mode. We recommend leaving the default 0.0 setting in place.

4. Auditory alert setting (beep)

The display will show F4 and then show whether the beep function is on or off. The default is ON. To turn it off, press the "-" button. Press the "+" button to turn the beep on. Press "⚙️" to advance to the backlight setting.

5. Setting the backlight

The display will show F5 and show whether backlight is on or off. The default is ON. To turn the backlight off, press the "-" button. Press the "+" button to turn the backlight back on. Press "⚙️" to exit the function setting mode. The display goes dark.

BEFORE TAKING A TEMPERATURE READING

Clean the skin of the forehead and make sure the area is free of hair, sweat, cream or makeup.


Wait at least 30 minutes after strenuous exercise to take your temperature.

Take the temperature in a room that does not have significant changes in air flow, such as a room with large fans and air conditioners. Do not take your temperature near heat sources, such as radiators or heat registers.

The body's temperature adapts to the environment. Allow at least 20 minutes to adjust to room temperature if a person is entering a room that is significantly warmer or cooler than the room they were in previously.

MEASURING FOREHEAD TEMPERATURE

Point the front of the thermometer (sensor head) at the center of the person's forehead, no more than 2 inches (5cm) away from the skin, and press the button on the handle. A beep indicates that the measurement is complete and the measurement value is shown on the display. In order to avoid human error, we suggest that you take multiple measurements at least 20 seconds apart and average them.

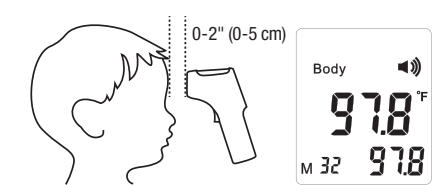

Fever Alerts

When the measured forehead temperature exceeds the preset fever threshold temperature, the thermometer will emit several beeps in a row, alerting you to a high temperature. The fever threshold temperature can be adjusted in the function settings (see above).

STORED READING RECALL

Turn the thermometer on by pressing the trigger button on the handle. The display lights up. The saved temperature readings (up to 32 readings) are displayed in the lower left-hand corner of the display (reading number) and the lower right hand corner (temperature). Press the "+" and "-" buttons, to move through the list of saved readings. Press and hold the +/- buttons to move through the list more quickly.

AUTOMATIC SHUT DOWN

This thermometer is equipped with a battery-saving automatic shutdown feature: after 15 seconds without any user action, the thermometer will power down. You can turn it back on by simply pressing the trigger button on the handle.

BATTERY REPLACEMENT

This product uses 2 AA alkaline batteries. When the display shows a battery icon, the batteries are low. To replace the batteries, push the battery cover on the bottom of the handle in the direction of the arrow. Take out the old batteries and install the new batteries, making sure the polarity is correct (note the "+" and "-" signs on the metal plate inside the battery door). Close the battery door and properly dispose of the batteries. If the thermometer is not used for more than 3 months, remove the batteries to prevent potential damage from battery fluid.

BATTERY SAFETY

1. This product requires 2 AA batteries.
2. Since batteries are sensitive to high temperatures, keep them in a cool, dry place when storing them.
3. Battery contacts need to be clean, both on the battery and in the appliance, before installation.
4. Batteries should be removed from the appliance when not being used for long periods of time (months).
5. Never recharge non-rechargeable batteries.
6. Use only the power cord supplied with the appliance.
7. Be careful to install (+) and (-) to the correct plus and minus on device.
8. Replace all old batteries at one time. Do not mix old and new.
9. Remove discharged batteries immediately to avoid leakage.
10. Never put batteries into a fire.
11. Switch off devices after use.
12. Keep batteries away from children, especially the batteries that are small enough to ingest.
13. If a battery is ingested, seek immediate medical help.
14. Never open, crush, puncture or disassemble batteries.
15. Dispose of batteries according to any state and Local regulations.
16. Do not dispose of rechargeable batteries as solid waste.